

HIGH STRENGTH & SAFETY

Double locking mechanism

INSTRUMENT-FREE


Fast & Easy implantation

CT/MRI ARTIFACT-FREE

100% PEEK-OPTIMA™

MINIMAL PROFILE

Guaranteed by 3D adaptation

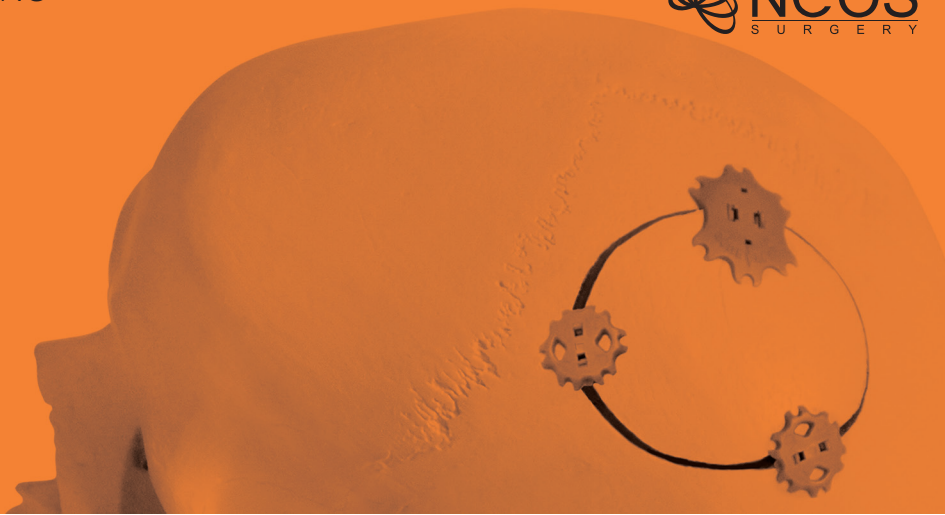

CRANIAL Loop (XL) BURR HOLE



REF: FC050200

- Burr hole device
- 22 mm diameter
- Profile: 0.9 mm

CRANIAL Loop (L)



REF: FC050100

- Osteotomy line device
- 16 mm diameter
- Profile: 1 mm

CRANIAL Loop



REF: FC050000

- Osteotomy line device
- 12 mm diameter
- Profile: 1 mm



Cranial LOOP was awarded the MDEA Gold distinction (NYC-USA)

CLINICAL AND FUNCTIONAL STUDIES


Asencio, C. *et al.* Long-Term Safety and Performance of a Polymeric Clamp-Like Cranial Fixation System. *World Neurosurg* 2019; 126: e758-e764

Van Loock, K. *et al.* "Cranial Bone Flap fixation using a New Device (Cranial Loop)", *Minim Invas Neurosurg* 2011; 54:119-124

Vilana, X. *et al.* "Comparison between PEEK and Titanium cranial fixation devices", *Proceedings of the 24th European Conference on Biomaterials* (September 2011, Dublin, Ireland).

INSTRUMENT-FREE

Savings in OR time, sterilisation and logistics

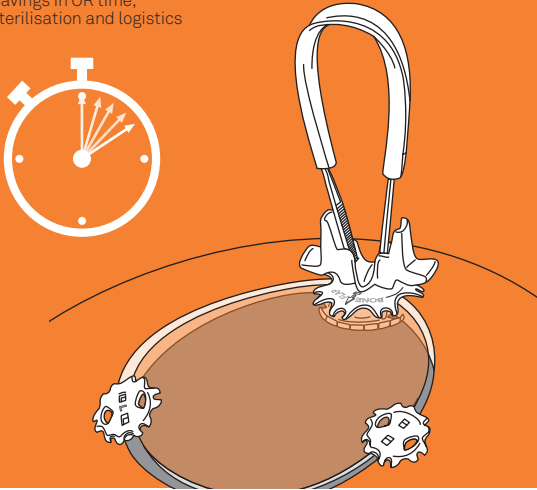


GENERAL INFORMATION


- Supplied ready to use: sterile, no instrument tray needed.
- Artifact-free in X-Ray, CT scan and MRI.
- Reduced risk of soft tissue damage due to the smart design and less aggressive material: PEEK-OPTIMA™.
- Can be used for bone thicknesses between 1.5 and 24 mm.
- Easy to remove using standard Neurosurgery forceps or rongeurs.
- PEEK-OPTIMA™ polymer is certified for implantation under ISO 10993 standards and US FDA Drug & DMF.
- CE-mark and FDA clearance.

NEOS SURGERY and Cranial LOOP are trademarks of NEOS SURGERY S.L.
PEEK OPTIMA™ is a trademark of Invivio Ltd.
Cranial LOOP is patented.

MINIMAL PROFILE



Before tightening




After tightening

CT/MRI ARTIFACT-FREE



Artifacts due to titanium device



Cranial LOOP artifact-free image

REINVENTING CRANIAL FIXATIONS


The Cranial LOOP family of cranial fixation devices are a smart system for securely fixing bone flaps resulting from craniotomies.

A fast and easy 'Pull and tighten' action allows the surgeon to control and feel the fixation. A standard bone flap with three Cranial LOOP devices can be fixed in less than a minute.

The different members of the Cranial LOOP family produce equivalent fixation strengths to those of other standard metallic NON-instrument-free fixation devices.




FORCE REQUIRED TO SINK THE BONE FLAP 2 mm

NEOS Surgery's data, based on the testing methodology by Dr. Lerch (Neurosurgery. 1999; 44 (4): 902-5)

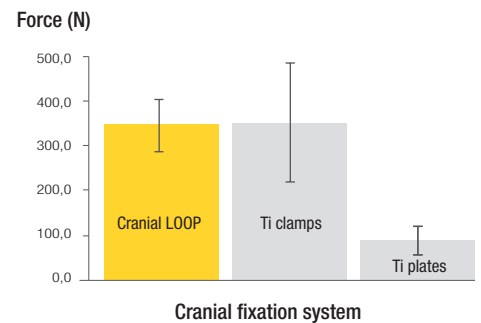

The Cranial LOOP family offers the safety of microplates and screws concerning brain tissue damage, combined with the ease of use and strength of clamping systems.

FAST & EASY

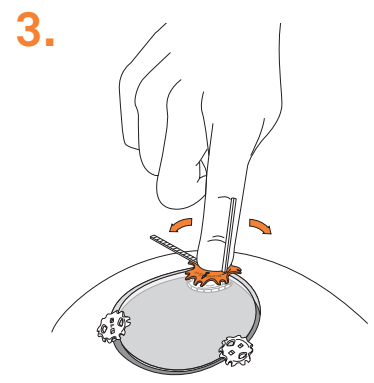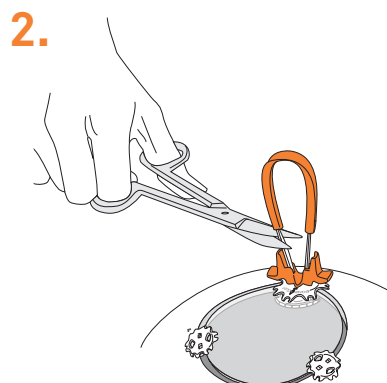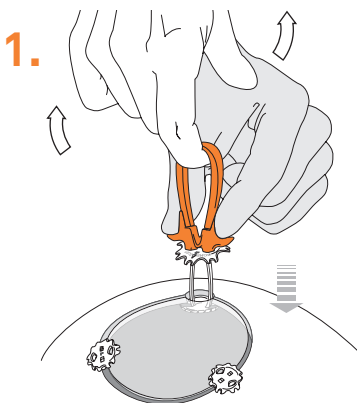

Distributed by:

Manufactured by:



NEOS SURGERY S.L.
www.neosurgery.com

C/Ceramistes, 2
08290 Cerdanyola del Vallès
(BARCELONA) - SPAIN

P. Mikeletegi, 2
20009 San Sebastián
(GUIPÚZCOA) - SPAIN